


Tue Sep 26 12:19:49 2006

TIDE Mass_0

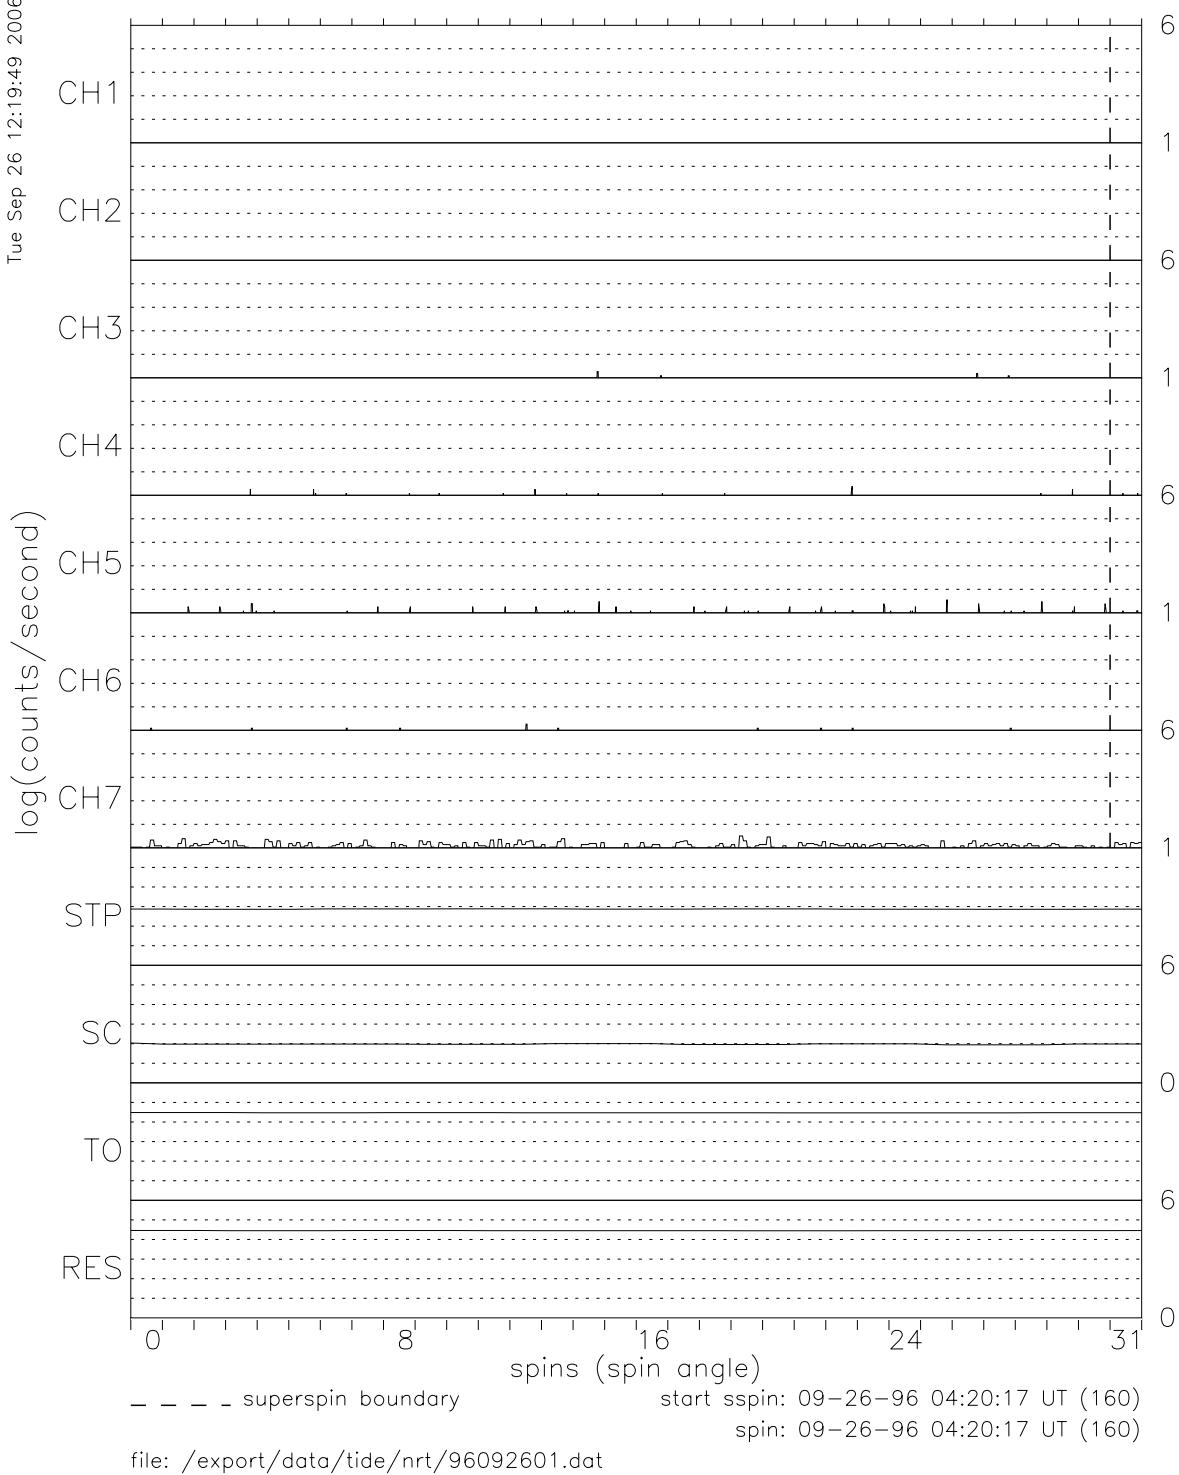

-15kV TOF: -9245 v

-3.6kV MCP: -2813 v

-2.4kV MCP: -1589 v


Input Cur: 304 ma

RPA max: 237 v

Mirror max: 238 v

Tue Sep 26 12:19:49 2006

TIDE Direct Events

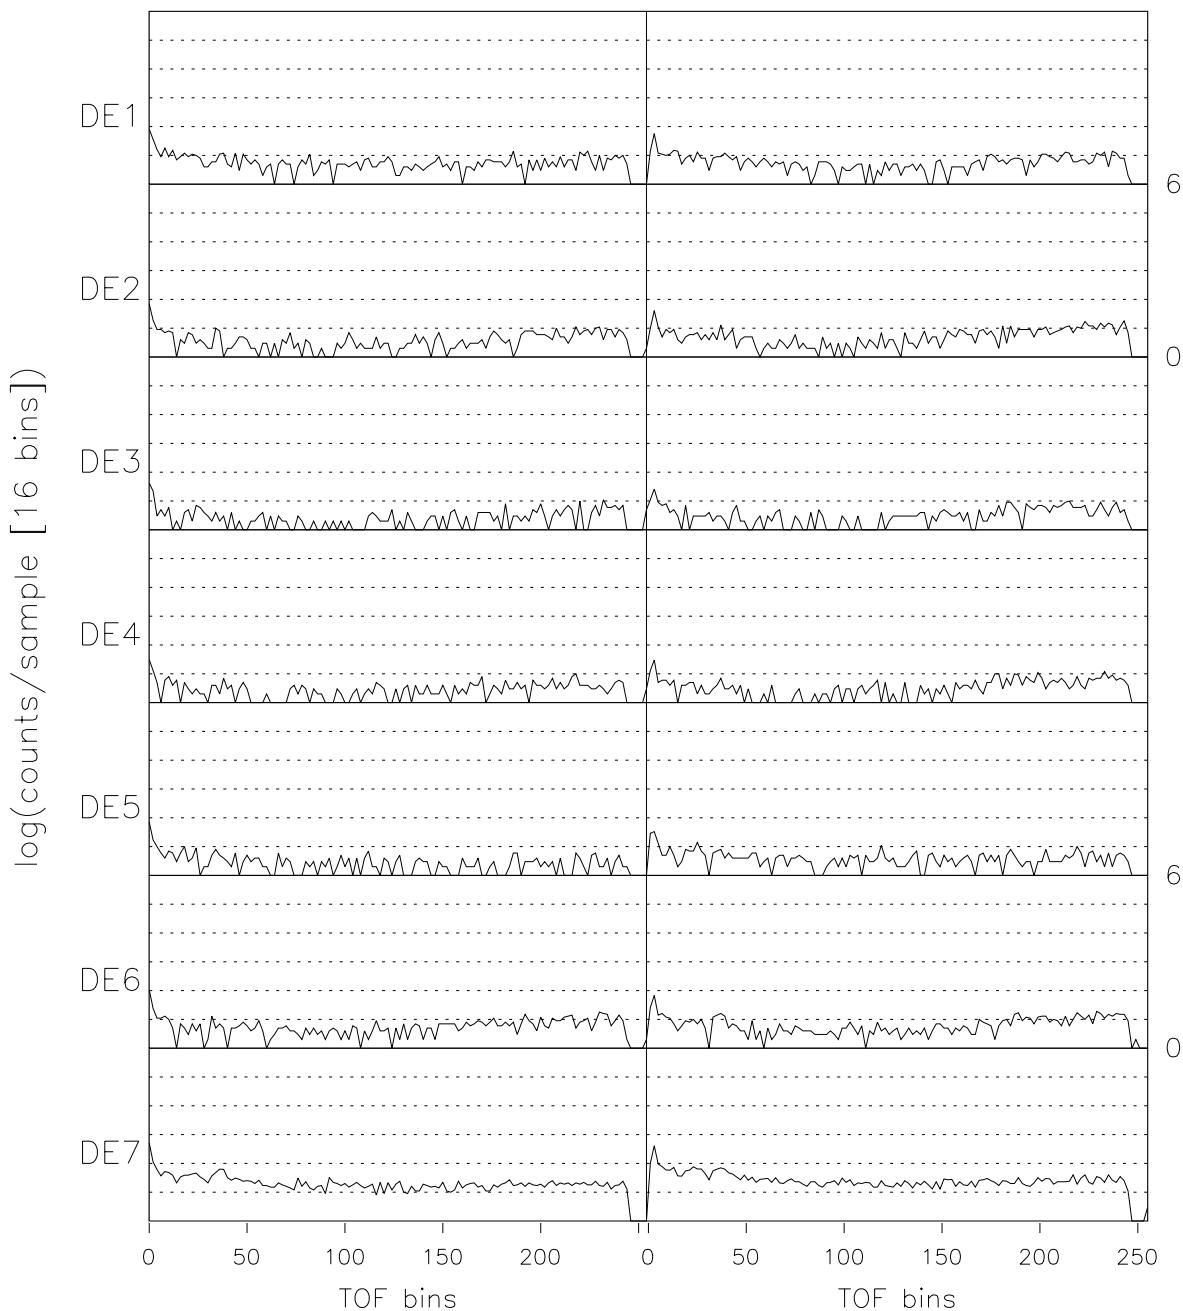

reported: 09-26-96 04:13:46 UT

reported: 09-26-96 04:16:58 UT

file: /export/data/tide/nrt/96092601.dat

-15kV TOF: -9116 v

-3.6kV MCP: -2782 v

-2.4kV MCP: -1579 v

Input Cur: 294 ma

RPA max: 237 v

Mirror max: 238 v